


# INSTRUCTION MANUAL

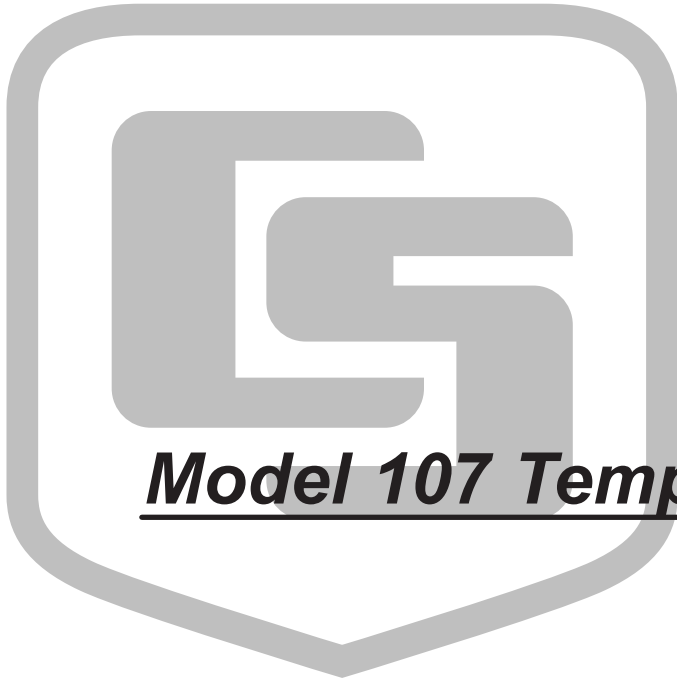

## *Model 107 Temperature Probe*

Revision: 7/04

Copyright (c) 1983-2004  
Campbell Scientific, Inc.

# **Warranty and Assistance**

---

The **MODEL 107 TEMPERATURE PROBE** is warranted by CAMPBELL SCIENTIFIC, INC. to be free from defects in materials and workmanship under normal use and service for twelve (12) months from date of shipment unless specified otherwise. Batteries have no warranty. CAMPBELL SCIENTIFIC, INC.'s obligation under this warranty is limited to repairing or replacing (at CAMPBELL SCIENTIFIC, INC.'s option) defective products. The customer shall assume all costs of removing, reinstalling, and shipping defective products to CAMPBELL SCIENTIFIC, INC. CAMPBELL SCIENTIFIC, INC. will return such products by surface carrier prepaid. This warranty shall not apply to any CAMPBELL SCIENTIFIC, INC. products which have been subjected to modification, misuse, neglect, accidents of nature, or shipping damage. This warranty is in lieu of all other warranties, expressed or implied, including warranties of merchantability or fitness for a particular purpose. CAMPBELL SCIENTIFIC, INC. is not liable for special, indirect, incidental, or consequential damages.

Products may not be returned without prior authorization. The following contact information is for US and International customers residing in countries served by Campbell Scientific, Inc. directly. Affiliate companies handle repairs for customers within their territories. Please visit [www.campbellsci.com](http://www.campbellsci.com) to determine which Campbell Scientific company serves your country. To obtain a Returned Materials Authorization (RMA), contact CAMPBELL SCIENTIFIC, INC., phone (435) 753-2342. After an applications engineer determines the nature of the problem, an RMA number will be issued. Please write this number clearly on the outside of the shipping container. CAMPBELL SCIENTIFIC's shipping address is:

**CAMPBELL SCIENTIFIC, INC.**

RMA# \_\_\_\_\_  
815 West 1800 North  
Logan, Utah 84321-1784

CAMPBELL SCIENTIFIC, INC. does not accept collect calls.

# 107 Table of Contents

---

*PDF viewers note: These page numbers refer to the printed version of this document. Use the Adobe Acrobat® bookmarks tab for links to specific sections.*

<b>1. General</b> .....	1
1.1 Specifications.....	1
<b>2. Accuracy</b> .....	1
<b>3. Installation and Wiring</b> .....	2
<b>4. Programming</b> .....	4
<b>5. Maintenance and Calibration</b> .....	6
<b>6. Instruction 11 Details</b> .....	6
<b>7. Electrically Noisy Environments</b> .....	8
<b>8. Long Lead Lengths</b> .....	9

## **Figures**

2-1. Error Produced by Polynomial fit to Published Values .....	2
3-1. 107 and 41303 Radiation Shield on a CM6/CM10 Tripod Mast.....	3
3-2. 107 Probe Datalogger Connections .....	4
6-1. 107 Thermistor Probe Schematic.....	8

## **Tables**

2-1. Thermistor Interchangeability Specification.....	2
2-2. Polynomial Error .....	2
3-1. Sensor Wiring.....	4
4-1. Wiring for Example 1 Program .....	4
4-2. Wiring for Example 2 Program .....	5
6-1. Temperature, Resistance, and Datalogger Output.....	7
6-2. Polynomial Coefficients .....	8



# Model 107 Temperature Probe

---

## 1. General

The 107 Temperature Probe uses a thermistor to measure temperature. Custom lead lengths are available up to 1000 ft.

The probe is designed for measuring air/soil/water temperatures. For air temperature, a 41303 radiation shield is used to mount the 107 Probe and limit solar radiation loading. The probe is designed to be buried or submerged in water to 50' (21 ps).

### 1.1 Specifications

Temperature

Measurement Range:  $-35^{\circ}$  to  $+50^{\circ}\text{C}$

Thermistor Inter-

changeability Error: Typically  $<\pm 0.2^{\circ}\text{C}$  over  $0^{\circ}\text{C}$  to  $60^{\circ}\text{C}$ ;  $\pm 0.4$  @  $-35^{\circ}\text{C}$

Temperature

Survival Range:  $-50^{\circ}\text{C}$  to  $+100^{\circ}\text{C}$

Polynomial

Linearization Error:  $<\pm 0.5^{\circ}\text{C}$  over  $-35^{\circ}\text{C}$  to  $+50^{\circ}\text{C}$

Time Constant

In Air: Between 30 and 60 seconds in a wind speed of  $5\text{ m s}^{-1}$

---

#### NOTE

The black outer jacket of the cable is Santoprene<sup>®</sup> rubber. This compound was chosen for its resistance to temperature extremes, moisture, and UV degradation. However, this jacket will support combustion in air. It is rated as slow burning when tested according to U.L. 94 H.B. and will pass FMVSS302. Local fire codes may preclude its use inside buildings.

---

## 2. Accuracy

The overall probe accuracy is a combination of the thermistor's interchangeability specification, the precision of the bridge resistors, and the polynomial error. In a "worst case" all errors add to an accuracy of  $\pm 0.4^{\circ}\text{C}$  over the range of  $-24^{\circ}$  to  $48^{\circ}\text{C}$  and  $\pm 0.9^{\circ}\text{C}$  over the range of  $-38^{\circ}\text{C}$  to  $53^{\circ}\text{C}$ . The major error component is the interchangeability specification of the thermistor, tabulated in Table 2-1. For the range of  $0^{\circ}$  to  $50^{\circ}\text{C}$  the interchangeability error is predominantly offset and can be determined with a single point calibration. Compensation can then be done with an offset entered in the measurement instruction. The bridge resistors are 0.1% tolerance with a 10 ppm temperature coefficient. Polynomial errors are tabulated in Table 2-2 and plotted in Figure 2-1.

TABLE 2-1. Thermistor Interchangeability Specification	
Temperature (°C)	Temperature Tolerance (±°C)
-40	0.40
-30	0.40
-20	0.32
-10	0.25
0 to +50	0.20

TABLE 2-2. Polynomial Error	
-40 to +56	<±1.0°C
-38 to +53	<±0.5°C
-24 to +48	<±0.1°C

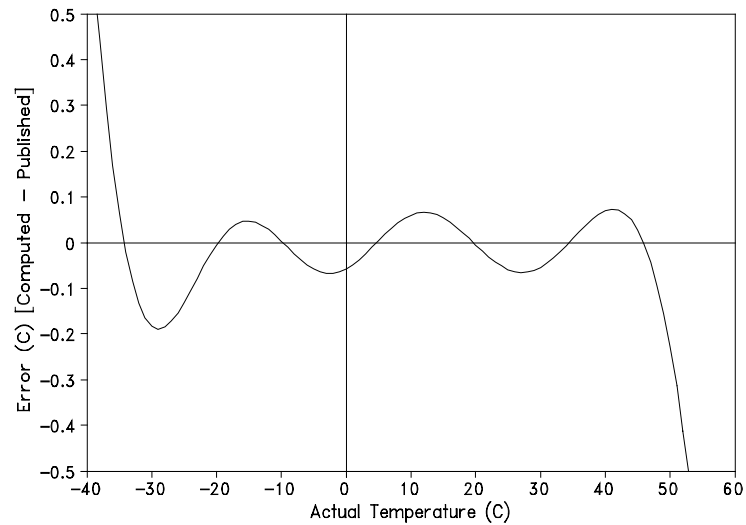


FIGURE 2-1. Error Produced by Polynomial Fit to Published Values

### 3. Installation and Wiring

For air temperature measurement, the 107 must be housed inside a radiation shield when used outdoors. The 41303 Radiation Shield (see Figure 3-1) mounts to a CM6 or CM10 tripod. The UT018 mounting arm and UT6P Radiation Shield mount to a UT30 tower.

The standard lead length of 6 feet and 9 feet allow the 107 to be mounted at a 2 meter height on the CM6/CM10 tripod or the UT30 tower respectively.

Connections to the datalogger for the 107 are shown in Figure 3-2 and Table 3-1.

The number of 107 probes per excitation channel is physically limited by the number of lead wires that can be inserted into a single excitation terminal (approximately 6).

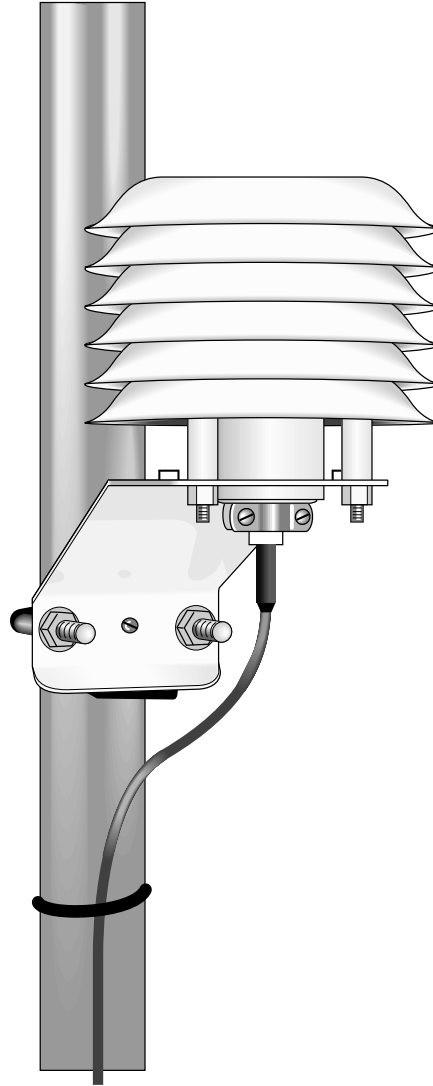


FIGURE 3-1. 107 and 41303 Radiation Shield on a CM6/CM10 Tripod Mast

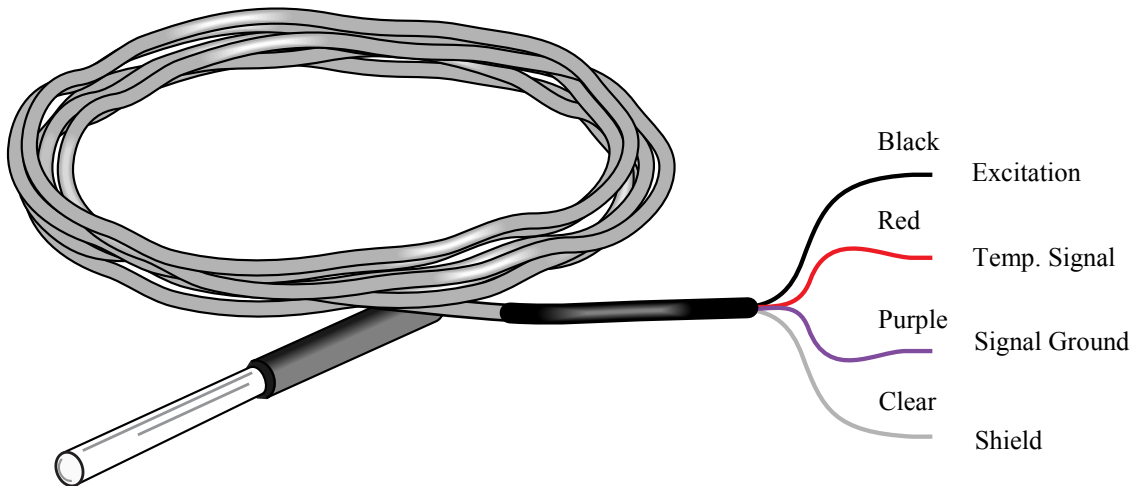


FIGURE 3-2. 107 Probe Datalogger Connections

Color	Function	CR10(X), CR510	21X, CR7, CR23X, CR1000
Black	Excitation	Switched Excitation	Switched Excitation
Red	Signal	Single-Ended Channel	Single-Ended Channel
Purple	Signal Ground	AG	⊕
Clear	Shield	G	⊕

## 4. Programming

In the CR1000 datalogger, Instruction Therm107 is used to measure temperature using a 107 temperature probe. Therm107 provides excitation, makes a single ended voltage measurement, and calculates temperature.

A multiplier of 1.0 and an offset of 0 yields temperature in Celsius. For Fahrenheit, use a multiplier of 1.8 and an offset of 32.

Color	Function	CR1000
Black	Excitation	Switched Ex Channel 1
Red	Signal	Single-Ended Channel 1
Purple	Signal Ground	⊕
Clear	Shield	⊕



**EXAMPLE 1. Sample Program for CR1000 Datalogger**

```
'CR1000
'This example program measures a single 107 Thermistor probe
'once a second and stores the average temperature every 10 minutes.

'Declare the variables for the temperature measurement
Public T107_C

'Define a data table for 10 minute averages:
DataTable(Table1,True,-1)
    DataInterval(0,10,Min,0)
    Average(1,T107_C,IEEE4,0)
EndTable

BeginProg
    Scan(1,Sec,1,0)
        'Measure the temperature
        Therm107(T107_C,1,1,Vx1,0,_60Hz,1.0,0.0)
        'Call Data Table
        CallTable(Table1)
    NextScan
EndProg
```

This section is for users who write their own datalogger programs. A datalogger program to measure this sensor can be created using Campbell Scientific's Short Cut Program Builder software. You do not need to read this section to use Short Cut.

Instruction 11 is used to measure temperature. Instruction 11 provides AC excitation, makes a single ended voltage measurement, and calculates temperature with a fifth order polynomial. A multiplier of 1.0 and an offset of 0.0 yields temperature in Celsius. For Fahrenheit, use a multiplier of 1.8 and an offset of 32.

**TABLE 4-2. Wiring for Example 2 Program**

Color	Function	CR10(X)
<b>Black</b>	Excitation	Switched Ex Channel 3
<b>Red</b>	Signal	Single-Ended Channel 9
<b>Purple</b>	Signal Ground	AG
<b>Clear</b>	Shield	G

**Example 2. Sample Program**

```
1: Temp (107) (P11)
  1:      1      Repts
  2:      9      SE Channel
  3:      3      Excite all reps w/E3
  4:      1      Loc [ Air_Temp ]
  5:      1.0    Mult
  6:      0.0    Offset
```

### Excitation/Integration Codes

Code	Result
0x	excite all rep with channel x
1x	increment chan x with each rep
2x	excite all reps with channel x, 60 Hz rejection, 10 ms delay
3x	excite all reps with channel x, 50 Hz rejection, 10 ms delay
4x	increment chan x with each rep, 60 Hz rejection, 10 ms delay
5x	increment chan x with each rep, 50 Hz rejection, 10 ms delay

## 5. Maintenance and Calibration

The 107 Probe requires minimal maintenance. Check monthly to make sure the radiation shield is free from debris.

For most applications it is unnecessary to calibrate the 107 to eliminate the thermistor offset. However, for those users that are interested, the following briefly describes calibrating the 107 probes.

A single point calibration can be performed to determine the 107 temperature offset (thermistor interchangeability). This calibration will not remove the polynomial error. The value of the offset must be chosen so that the probe outputs the temperature calculated by the polynomial, not the actual calibration temperature. For example, a 107 is placed in a calibration chamber that is at 0°C and the probe outputs 0.1°C. The offset is -0.16, because at 0°C the polynomial calculates a temperature of -0.06°C (Table 6-1).

## 6. Instruction 11 Details

Understanding the details in this section are not necessary for general operation of the 107 Probe with CSI's dataloggers.

Instruction 11 outputs a precise 2 VAC excitation (4 V with the 21X) and measures the voltage drop due to the sensor resistance (Figure 6-1). The thermistor resistance changes with temperature. Instruction 11 calculates the ratio of voltage measured to excitation voltage ( $V_s/V_x$ ) which is related to resistance, as shown below:

$$V_s/V_x = 1000/(R_s+249000+1000)$$

where  $R_s$  is the resistance of the thermistor.

See the measurement section of the datalogger manual for more information on bridge measurements.

Instruction 11 then calculates temperature using a fifth order polynomial equation correlating  $V_s/V_x$  with temperature. The polynomial coefficients are given in Table 6-2. The polynomial input is  $(V_s/V_x)*800$ . Resistance and datalogger output at several temperatures are shown in Table 6-1.

**TABLE 6-1. Temperature, Resistance,  
and Datalogger Output**

<b>Temperature °C</b>	<b>Resistance OHMS</b>	<b>Output °C</b>
-40.00	4067212	-39.18
-38.00	3543286	-37.55
-36.00	3092416	-35.83
-34.00	2703671	-34.02
-32.00	2367900	-32.13
-30.00	2077394	-30.18
-28.00	1825568	-28.19
-26.00	1606911	-26.15
-24.00	1416745	-24.11
-22.00	1251079	-22.05
-20.00	1106485	-20.00
-18.00	980100	-17.97
-16.00	869458	-15.95
-14.00	772463	-13.96
-12.00	687276	-11.97
-10.00	612366	-10.00
-8.00	546376	-8.02
-6.00	488178	-6.05
-4.00	436773	-4.06
-2.00	391294	-2.07
0.00	351017	-0.06
2.00	315288	1.96
4.00	283558	3.99
6.00	255337	6.02
8.00	230210	8.04
10.00	207807	10.06
12.00	187803	12.07
14.00	169924	14.06
16.00	153923	16.05
18.00	139588	18.02
20.00	126729	19.99
22.00	115179	21.97
24.00	104796	23.95
26.00	95449	25.94
28.00	87026	27.93
30.00	79428	29.95
32.00	72567	31.97
34.00	66365	33.99
36.00	60752	36.02
38.00	55668	38.05
40.00	51058	40.07
42.00	46873	42.07
44.00	43071	44.05
46.00	39613	46.00
48.00	36465	47.91
50.00	33598	49.77
52.00	30983	51.59
54.00	28595	53.35
56.00	26413	55.05
58.00	24419	56.70
60.00	22593	58.28

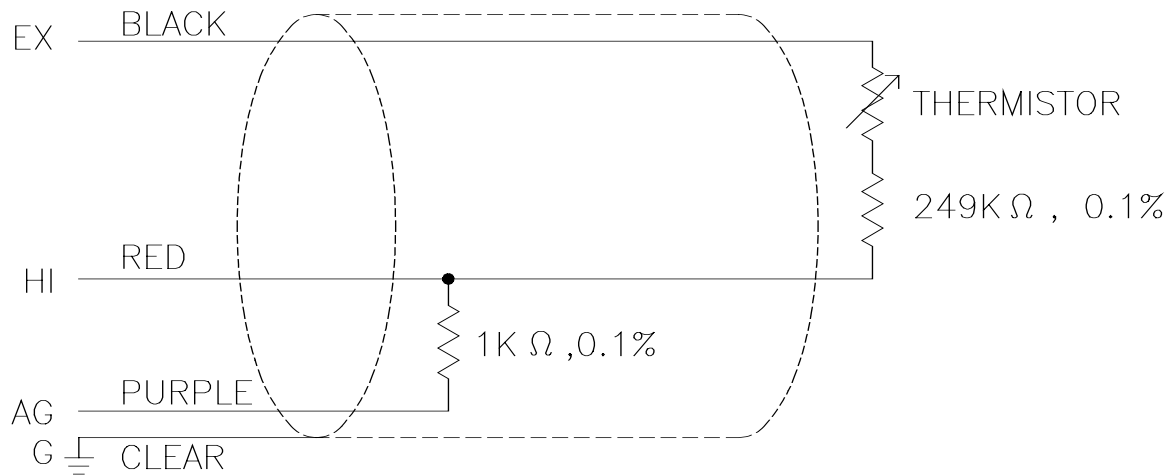


FIGURE 6-1. 107 Thermistor Probe Schematic

Coefficient	Value
C0	-53.4601
C1	90.807
C2	-83.257
C3	52.283
C4	-16.723
C5	2.211

## 7. Electrically Noisy Environments

AC power lines can be the source of electrical noise. If the datalogger is in an electronically noisy environment, the 107 temperature measurement should be measured with 60 Hz rejection. Sixty and 50 Hz rejection is available as an option in the Excitation Channel parameter of Instruction 11 for the CR10X, CR510, and CR23X dataloggers. For the CR10, CR21X and CR7, the 107 should be measured with the AC half bridge (Instruction 5).

### Example 3. Sample CR10(X) Instructions Using AC Half Bridge

1: AC Half Bridge (P5)		
1:	1	Reps
2:	22	7.5 mV 60 Hz Rejection Range
3:	9	SE Channel
4:	3	Excite all reps w/Exchan 3
5:	2000	mV Excitation ;Use 4000 mV on 21X and CR7
6:	1	Loc [ Air_Temp ]
7:	800	Mult
8:	0	Offset

2: Polynomial (P55)		
1:	1	Reps
2:	1	X Loc [ Air_Temp ]
3:	1	F(X) Loc [ Air_Temp ]
4:	-53.46	C0
5:	90.807	C1
6:	-83.257	C2
7:	52.283	C3
8:	-16.723	C4
9:	2.211	C5

## 8. Long Lead Lengths

The 60 and 50 Hz rejection options for the CR10X, CR510, and CR23X include a delay to accommodate long lead lengths. For the CR10, 21X, and CR7, if the 107 has lead lengths of more than 300 feet, use the DC Half Bridge instruction (Instruction 4) with a 2 millisecond delay to measure temperature. The delay provides a longer settling time before the measurement is made. Do not use the 107 with long lead lengths in an electrically noisy environment.

### Example 4. Sample Program CR10 Using DC Half Bridge with Delay

1: Excite-Delay (SE) (P4)		
1:	1	Reps
2:	2	7.5 mV Slow Range
3:	9	SE Channel
4:	3	Excite all reps w/Exchan 3
5:	2	Delay (units 0.01 sec)
6:	2000	mV Excitation ;Use 4000 mV on 21X and CR7
7:	1	Loc [ Air_Temp ]
8:	.4	Mult ;Use 0.2 on 21X and CR7
9:	0	Offset
2: Polynomial (P55)		
1:	1	Reps
2:	1	X Loc [ Air_Temp ]
3:	1	F(X) Loc [ Air_Temp ]
4:	-53.46	C0
5:	90.807	C1
6:	-83.257	C2
7:	52.283	C3
8:	-16.723	C4
9:	2.211	C5





## **Campbell Scientific Companies**

---

### **Campbell Scientific, Inc. (CSI)**

815 West 1800 North  
Logan, Utah 84321  
UNITED STATES  
[www.campbellsci.com](http://www.campbellsci.com)  
[info@campbellsci.com](mailto:info@campbellsci.com)

### **Campbell Scientific Africa Pty. Ltd. (CSAf)**

PO Box 2450  
Somerset West 7129  
SOUTH AFRICA  
[www.csafrica.co.za](http://www.csafrica.co.za)  
[sales@csafrica.co.za](mailto:sales@csafrica.co.za)

### **Campbell Scientific Australia Pty. Ltd. (CSA)**

PO Box 444  
Thuringowa Central  
QLD 4812 AUSTRALIA  
[www.campbellsci.com.au](http://www.campbellsci.com.au)  
[info@campbellsci.com.au](mailto:info@campbellsci.com.au)

### **Campbell Scientific do Brazil Ltda. (CSB)**

Rua Luisa Crapsi Orsi, 15 Butantã  
CEP: 005543-000 São Paulo SP BRAZIL  
[www.campbellsci.com.br](http://www.campbellsci.com.br)  
[suporte@campbellsci.com.br](mailto:suporte@campbellsci.com.br)

### **Campbell Scientific Canada Corp. (CSC)**

11564 - 149th Street NW  
Edmonton, Alberta T5M 1W7  
CANADA  
[www.campbellsci.ca](http://www.campbellsci.ca)  
[dataloggers@campbellsci.ca](mailto:dataloggers@campbellsci.ca)

### **Campbell Scientific Ltd. (CSL)**

Campbell Park  
80 Hathern Road  
Shepshed, Loughborough LE12 9GX  
UNITED KINGDOM  
[www.campbellsci.co.uk](http://www.campbellsci.co.uk)  
[sales@campbellsci.co.uk](mailto:sales@campbellsci.co.uk)

### **Campbell Scientific Ltd. (France)**

Miniparc du Verger - Bat. H  
1, rue de Terre Neuve - Les Ulis  
91967 COURTABOEUF CEDEX  
FRANCE  
[www.campbellsci.fr](http://www.campbellsci.fr)  
[campbell.scientific@wanadoo.fr](mailto:campbell.scientific@wanadoo.fr)

### **Campbell Scientific Spain, S. L.**

Psg. Font 14, local 8  
08013 Barcelona  
SPAIN  
[www.campbellsci.es](http://www.campbellsci.es)  
[info@campbellsci.es](mailto:info@campbellsci.es)